



Instructions for Use

HICO-AQUATHERM 660



CE 0598

pfm medical hico gmbh

Wankelstraße 60

50996 Köln, Germany

Tel.: +49 (0) 2 21 / 37 67 8 - 0

Fax: +49 (0) 2 21 / 37 67 8 - 85

Email: hico@pfmmedical.com

Internet: www.hico.de

Material Number GA-592801-EN

Version: 05

valid from: 2024-07-05

© 2024 pfm medical hico gmbh

1	General information.....	6
1.1	Information regarding these instructions	6
1.2	Warnings.....	7
1.3	Limitation of liability	8
1.4	Copyright.....	8
1.5	Manufacturer’s address.....	8
2	Safety	9
2.1	Intended use	9
2.1.1	Intended use environment	9
2.1.2	Patient Population.....	9
2.1.3	Intended user	9
2.2	Personnel requirements.....	10
2.3	General safety instructions	11
2.4	Potential hazards	13
2.4.1	Danger of the hyperthermia.....	13
2.4.2	Risk of burns.....	13
2.4.3	Risk of chemical substances.....	13
3	Transport and setup.....	14
3.1	Scope of delivery and transport inspection	14
3.2	Unpacking	14
3.3	Disposal of the packaging material.....	15
4	Commissioning	16
4.1	Safety instructions	16
4.2	Setup.....	16
4.2.1	Requirements on the installation site / operating location.....	16
4.2.2	Mounting on a wall rail (optional)	18
4.2.3	Installation with five-castor stand (optional).....	18
4.3	Connecting the HICO-AQUATHERM 660	19
4.3.1	Filling the system.....	19
4.3.2	Connecting the water pads	20
4.3.3	Electrical connection	21
5	Design and function.....	22
5.1	Views of the unit, control elements, and display elements.....	22
5.2	Safety devices	23
5.2.1	Sensors	23
5.3	Symbols	24

5.4	Function	25
5.4.1	Basic principles	25
5.4.2	Indications / contraindications / side effects	27
6	Control and operation	30
6.1	Before switching on	30
6.1.1	Check the unit	30
6.1.2	Water pads	30
6.1.3	Heat output	31
6.2	Operation.....	32
6.2.1	Switching on for the first time	32
6.2.2	Switching on in normal operation	32
6.2.3	Functional test.....	33
6.2.4	Setting the temperature	34
6.2.5	Temperature control mode	36
6.2.6	Handling water pads.....	37
6.2.7	Using water pads.....	37
6.2.8	Schematic performance charts	38
6.2.9	Responsibilities during operation	41
6.2.10	Operating language	43
6.3	Alarms.....	44
6.3.1	General information	44
6.3.2	Description of alarms during operation	44
7	Cleaning and disinfection	48
7.1	Safety instructions	48
7.2	Unit	49
7.2.1	Water circuit	49
7.2.1.1.	General Information for cleaning the water circuit.....	49
7.2.1.2.	Basic cleaning.....	49
7.2.1.3.	Disinfection.....	49
7.2.1.4.	Flushing and refilling.....	50
7.2.2	Surfaces	50
7.2.3	Ventilation slots.....	50
7.3	Water pads, hose extension.....	52
8	Maintenance and safety check.....	53
8.1	Maintenance	53
8.1.1	Unit.....	54
8.1.2	Water tank	54

8.1.3	Hose connections	54
8.2	Safety check	55
8.2.1	Standard configuration for the safety check.....	55
9	Troubleshooting	57
9.1	Safety instructions	57
9.2	Causes of error and troubleshooting	58
10	Disposal of an old unit.....	60
11	Technical data, unit, and accessories.....	61
11.1	Unit	61
11.2	Accessories.....	62
12	Guidelines and manufacturer's declaration	64
13	Quick Start Guide.....	68

1 General information

Please read the information in this manual to become acquainted with the HICO-AQUATHERM 660 as quickly as possible and to be able to utilise its functions to the full extent.

1.1 Information regarding these instructions

These instructions for use are a component of the HICO-AQUATHERM 660 (referred to in the following as the “unit”) and provide important information for the commissioning, safety, proper use, and maintenance of the unit.

All figures and drawings in these instructions for use are for general illustration purposes and are not definitive in terms of the details of the construction of the units.

The instructions for use must always be available, preferably in the vicinity of the unit. They must be read and applied by all persons who are responsible for the following:

- Commissioning
- Operation
- Cleaning
- Maintenance
- Troubleshooting

1.2 Warnings

The following types of safety notes are used in these instructions for use:

▲ DANGER

A DANGER note identifies an imminent danger situation.

Failure to avoid such a dangerous situation will cause severe injury or even death.

- ▶ Follow the instructions given in this danger note to avoid the danger of death or severe injury to people.

▲ WARNING

A WARNING note identifies a potentially dangerous situation.

Failure to avoid such a dangerous situation can lead to severe injuries.

- ▶ Follow the instructions in this warning note to avoid the risk of personal injury.

▲ CAUTION

A CAUTION note identifies a potentially dangerous situation or a risk of property damage.

Failure to avoid such a dangerous situation can lead to minor or moderate injuries and damage to property.

- ▶ Follow the instructions in this caution note to avoid the risk of personal injury and damage to property.

NOTE

A note highlights additional information to assist you when working with the unit.

1.3 Limitation of liability

All technical information, data, and notes on operation and maintenance contained in this manual were up-to-date at the time of printing and are provided to the best of our knowledge based on our previous knowledge and experience.

No claims can be derived on the basis of information, illustrations, or descriptions provided in these operating instructions.

The manufacturer accepts no responsibility for loss in the event of:

- Failure to follow the operating instructions
- Improper use
- Improper repairs
- Technical modifications
- The use of non-approved spare parts or non-approved accessories
- Unauthorised conversions and changes

Please inform us immediately of any serious incidents involving our product. If you are located in the EU, please also report the incident to the authorised representative as well as the competent authority of the Member State.

1.4 Copyright

This documentation is protected by copyright law.

All rights, also the rights for photo-mechanical reproduction, duplication, and distribution by means of special methods (e.g. data processing, data media, and data networks), even in parts, are reserved by the pfm medical hico gmbh.

Technical data and content subject to change without notice.

1.5 Manufacturer's address

pfm medical hico gmbh

Wankelstraße 60

50996 Köln, Germany

Tel.: +49 (0)2 21 / 3 76 78-0

Fax: +49 (0)2 21 / 3 76 78-85

Email: hico@pfmmedical.com

2 Safety

This chapter contains important safety information for working with this unit.

This unit complies with the specified safety regulations. However, improper use can lead to personal injury or property damage.

2.1 Intended use

The device is intended for patient temperature management in combination with hico qualified water pads without monitoring the body temperature.

▲ WARNING

Danger due to improper use!

It is dangerous to use the unit improperly and/or use the unit for any other purpose than the described purpose.

- ▶ Only use the unit for its intended purpose.
- ▶ Follow the procedures described in these instructions for use.
- ▶ Use only with original accessories.

Claims of any type due to damage resulting from improper use are excluded. The owner is the sole bearer of the risk.

2.1.1 **Intended use environment**

Only clinical use, the patient must be monitored during use, e.g. operating theatre and intensive care unit. Outpatient use is excluded.

The applied parts should be used for external application on the patient.

2.1.2 **Patient Population**

The patient population arises from the need to control the body temperature during treatment in intensive care units, burn centres, emergency departments and operating rooms.

2.1.3 **Intended user**

Use only by trained staff with appropriate specialist knowledge and training, e.g. anesthetists, anesthesiologists, intensive care and operating room nurses, surgeons and medical technicians.

2.2 Personnel requirements

NOTE

- ▶ Work on/with the unit may only be carried out by persons who are authorised for this work because of their education and qualifications. In addition, these persons must be authorised to perform the work by the owner.
- ▶ Personnel who will be trained, taught, instructed, or who are undergoing general training to work on or with the unit, are only allowed to work with the unit under the constant supervision of an experienced person.
- ▶ Persons who are under the influence of drugs, alcohol, or medication that affects their responsiveness may under no circumstances carry out work on or with the unit.
- ▶ Hazards can result when the unit is used improperly by untrained personnel.
- ▶ In addition to the instructions for use, all generally valid legal and otherwise binding regulations for the prevention of accidents and protection of the environment as well as general safety and performance requirements must be followed. The owner must instruct his personnel accordingly.

2.3 General safety instructions

NOTE

Follow the general safety instructions below for safe handling of the unit:

- ▶ Ensure that the unit (mains cable, housing, couplings, etc.), hoses, and water pads are in good condition before commissioning.
- ▶ Do not sit or stand on the unit.
- ▶ Lay hoses and water pads without creases and kinks.
- ▶ Do not touch the hoses and water pads with pointed or sharp objects. The system cannot work correctly with perforated pads.
- ▶ Fill the unit's tank with sterile filtered tap water¹ to which a disinfectant² has been added.
- ▶ Only operate the unit after the tank has been closed by screwing on the cap.
- ▶ Set up and operate the device horizontally; slope of the installation surface $\leq 3\%$.
- ▶ Height difference between the unit and water pad < 1 m.
- ▶ Do not cover unit. There are ventilation openings on the bottom and back of the unit.
- ▶ Monitor the automatic functional test when switching the unit on.
- ▶ Perform an automatic functional test manually at least once a day during continuous operation.
- ▶ Electrical medical devices are subject to special precautionary measures in terms of EMC³ and must be put into operation according to EMC instructions included in instructions for use.
- ▶ Portable and mobile RF communications equipment can affect medical electrical equipment.

¹ Depending on the quality of the water (e.g. its hardness, among other things), the lifetime of the parts of the unit that come into contact with water may be reduced.

² For example 10 ml SANOSIL mixture (from Sanosil, Farchant) \Rightarrow (1000 ml sterile filtered tap water + 10 ml Sanosil solution). If you have any questions, please contact the Customer Service department of pfm medical hico gmbh. The use of a disproportionately high amount of disinfectant can reduce the lifetime of parts of the unit that come into contact with water. The use of too much disinfectant can also immediately cause malfunctions, for example due to the excessive formation of foam!

³ Electromagnetic compatibility

- ▶ During operation, check the water flow and the water level in the unit at regular intervals.
- ▶ Only operate the unit with an appropriate water level.
- ▶ Stay within the ambient temperature range (10-30 °C) and storage temperature range (3-60 °C).
- ▶ Apply appropriate measures to position the patient on or under the water pad (if necessary).
- ▶ Do not use water pads as electrical insulation pads in combination with HF surgery.
- ▶ Intermediate layers between the patient and water pad (bed sheets, surgical drapes, gel pads, etc.) adversely affect the heat transfer.
- ▶ Only operate the unit with water pads qualified by HICO and original accessories.
- ▶ Do not operate the unit in an oxygen-enriched environment or in the presence of combustible gases.
- ▶ In hyperthermia mode, do not use or combine the unit together with other heat sources.
- ▶ Do not operate the unit in the vicinity of heat sources (spotlights, direct sunlight, radiators, radiant heaters, etc.).
- ▶ Perform maintenance and conduct safety checks according to these instructions for use.

2.4 Potential hazards

2.4.1 Danger of the hyperthermia

▲ WARNING

There is a risk of the patient becoming overheated.

- ▶ The patient's body temperature must be monitored when using the unit and water pad on the patient.

2.4.2 Risk of burns

▲ WARNING

HF surgery can cause burns

- ▶ To ensure that patients are not burned accidentally when using monopole HF tools on grounded conductive parts that are in contact with the patient, make sure that the opposing electrode is properly fastened.

2.4.3 Risk of chemical substances

▲ WARNING

- ▶ Some of the alloys used in the components of this device contain small amounts of lead for improved machining. The lead is, however, firmly bound in the metal matrix. When used as intended, the lead in the alloys is not released and does not represent any risk to the user. As an additional precaution, we recommend that you wear gloves when changing the HICO-Hose extension and connecting the equipotential bonding bolt.

3 Transport and setup

3.1 Scope of delivery and transport inspection

The scope of delivery of the HICO-AQUATHERM 660 consists of:

- HICO-AQUATHERM 660 unit
- Power cable (3 meters)
- Hose holder
- Instructions for Use
- Hose extension

NOTE

- ▶ Check the delivery for completeness and for any visible damage.
- ▶ Immediately report an incomplete delivery or damage caused by inappropriate packaging or transport to the forwarding agent, the insurance company, and the supplier.

3.2 Unpacking

To unpack the unit:

- Take the unit out of its box and remove the packaging material.
- Place the unit on a smooth, level surface with sufficient load bearing capacity.

▲ CAUTION

Condensation in the unit can lead to failure of the unit.

- ▶ After unpacking, the unit must be acclimatised for at least two hours before commissioning when the actual ambient temperature differs from the specified ambient temperature by more than 8 °C.

3.3 Disposal of the packaging material



The packaging protects the unit from damage during transport. The packaging materials are selected on the basis of environmentally friendly and disposal-related factors and are therefore recyclable.

Returning the packaging material back into the material cycle saves raw materials and decreases the amount of waste produced. Dispose of packaging materials that are no longer required at the collection points for the “Green Dot” recycling system or of your local recycling system.

NOTE

- ▶ If possible, keep the original packaging throughout the unit’s lifetime so that you can repack the unit properly in case of repair.
- ▶ If the original packaging is not available anymore, then you can request it from the manufacturer.

4 Commissioning

This chapter contains important instructions for commissioning the unit. Please follow these instructions to avoid danger and prevent damage.

4.1 Safety instructions

▲ WARNING

Injuries and property damage can occur when commissioning the unit!

Follow the safety instructions below to prevent hazardous situations:

- ▶ The weight of the unit is approx. 7 kg.
- ▶ The unit should only be transported, unpacked, and installed by two people or more.
- ▶ Do not use the unit directly next to or stacked on top of other equipment.
- ▶ If it is necessary to operate the unit directly next to other equipment in spite of this, then it is necessary to monitor the unit to ensure that it is being used for its intended purpose.

4.2 Setup

4.2.1 Requirements on the installation site / operating location

For safe and trouble-free operation of the unit, the installation site must fulfil the following requirements:

- It must have sufficient load bearing capacity (weight of unit approx. 7 kg).
- It must be level.
- It must be horizontal (slope $\leq 3\%$).
- It must provide 20 cm space on the back of the unit.
- It must ensure adequate ventilation of the unit, including upward ventilation in an equipment trolley.
- It must be at the same level as the water pad, i.e. next to the patient's bed (max. height difference approx. 1 m), for example.

The five-castor stand (see section 4.2.3) available as accessory meets all of these requirements. Make sure that all important parts of the unit (switches, power cable, hose connections, etc.) are easily accessible.

NOTE

- ▶ If the unit is not horizontal, then the display on the front of the unit will display the water level incorrectly.
- ▶ If the unit is far below the level of the water pad, then the circulation of water may be interrupted when the patient is heavy. Furthermore, water may flow back into the unit and cause the water tank to overflow when the water filling neck is open and the unit is switched off.

For optimal operation of the unit, the installation site should meet the following environmental conditions:

- Ambient temperature: 10 °C to 30 °C
- Relative humidity: 30 % to 70 %
- Air pressure: 700 hPa to 1060 hPa

▲WARNING


Performance limitations in terms of the attainable pad transition temperatures under extreme ambient conditions or due to the combination of pads selected (see section 6.2.8 “Schematic performance charts”) may also lead to restrictions in the scope its intended purpose.

▲CAUTION

Condensation in the unit can lead to failure of the unit.

- ▶ After unpacking, the unit must be acclimatised for at least two hours before commissioning when the actual ambient temperature differs from the specified ambient temperature by more than 8 °C.

4.2.2 Mounting on a wall rail (optional)

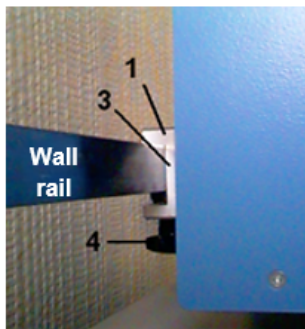


The unit can be mounted on wall rails (25 x 10 mm) typically found in clinics. For this purpose, fasten the clamp holder (1) (available as an accessory) on the back panel of the unit using two screws (3).

Use the star knob (4) on the clamp holder to fasten the unit to the rail.

4.2.3 Installation with five-castor stand (optional)

The five-castor stand available as an accessory can be used to move the HICO-AQUATHERM 660, which was designed as a stationary unit, to its location of use.

Install the unit together with the stand as follows:

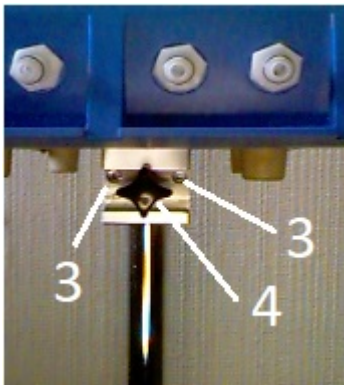

- Assemble the five-castor stand as described in its operating instructions.
- Fasten the clamp holder (1) (available as an accessory) to the five-castor stand in the required position on the bottom of the unit using the two screws (3).
- Place the HICO-AQUATHERM 660 on the cylinder (2) of the five-castor stand.
- Fasten the unit in place using the star knob (3).



⚠ CAUTION

Injuries and property damage may occur when installing and using the five-castor stand with the unit!

- ▶ When assembling the stand, follow the safety instructions in the assembly instructions and instructions for use for the stand!
- ▶ If a defect is detected, use only original spare parts as replacements and only allow parts to be replaced by a specialist or customer service.


4.3 Connecting the HICO-AQUATHERM 660

⚠ WARNING

Danger due to water in connection with electricity.

- ▶ Only connect the unit to the mains supply after it has been filled.

4.3.1 Filling the system

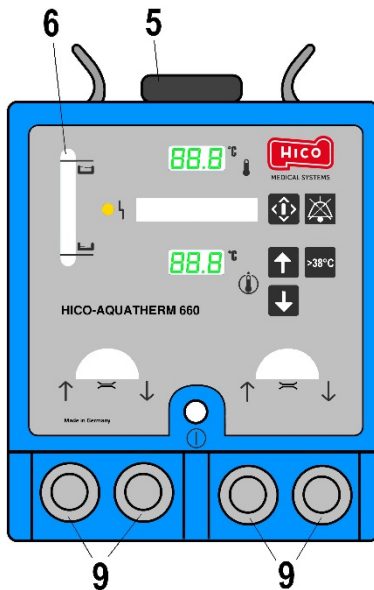

- Unscrew the cap from the water filling neck (5), e.g. with a coin. Take care not to lose the seal ring of the cap.
- Observe the water level indicator (6) while filling. After filling, the water level should be slightly below the MAX mark.
- Fill the unit with sterile filtered tap water⁴ to which a disinfectant⁵ has been added.
- After filling, screw the cap hand-tight back onto the water filling neck until it is properly sealed.

NOTE

The use of a disproportionately high amount of disinfectant can reduce the lifetime of parts of the unit that come into contact with water. When filling the unit for the first time, please follow the procedure described in section 6.2.1.

⚠ WARNING

Danger due to water in connection with electricity.

Water conducts electricity.


- ▶ If water overflows when filling the unit, then the unit must first be thoroughly dried and should only be connected to the mains supply and switched on after it has completely dried out.

⁴ Depending on the quality of the water (e.g. its hardness, among other things), the lifetime of the parts of the unit that come into contact with water may be reduced.

⁵ For example 10 ml SANOSIL mixture (from Sanosil, Farchant) ⇒ (1000 ml sterile filtered tap water + 10 ml Sanosil solution). If you have any questions, please contact the Customer Service department of pfm medical hico gmbh.

The use of a disproportionately high amount of disinfectant can reduce the lifetime of parts of the unit that come into contact with water! The use of too much disinfectant can also immediately cause malfunctions, for example due to the excessive formation of foam!³

4.3.2 Connecting the water pads

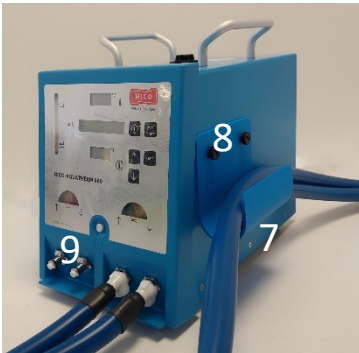

- The hose holder (7) provided makes it easier to lay the hoses between the pad and the unit. To attach the holder to the right-hand side of the unit, use the two knurled thumb screws (8) supplied with the unit.
- Push the hose connectors of a HICO hose extension onto the left or right hose connections (9) on the unit.
- Push the hose pad connectors of the hose extension onto the two hose connections on the water pad.
- The connectors are properly connected to each other when the locking mechanisms on the connectors engage their corresponding counterparts so that the connection will no longer come loose by itself.
- You can disconnect the hoses from the unit by pushing the metal plate on the hose connector and then pulling out the connector.

NOTE

- ▶ The hose extension connections cannot be “confused” when connecting them to the unit because it makes no difference which direction the water flows through the water pad.
- ▶ Water pads can also be disconnected when the unit is switched on. It is normal in this case for water to drip out of the connector and does not indicate leakage or a defect.
In the heating mode at 39 °C: Reduce the nominal temperature before disconnecting the water pad. Otherwise the water in the unit’s circuit can briefly rise above the upper temperature limit, and the unit may trigger various alarms.

4.3.3 Electrical connection

▲ CAUTION

Hazard due to electrical current

Defective cables and/or plugs as well as faults in the power supply can cause life-threatening electric shock!

- ▶ Check the condition of the unit's cables and plugs before connecting!
- ▶ To avoid the risk of electric shock, this unit must only be connected to a mains connection with a protective conductor!
- ▶ To safely disconnect the device from power in case of a malfunction, unplug the power cable from the mains socket. Make sure that the mains power connection on the rear of the device is easy to access.

Please follow the instructions below when making the electrical connections to ensure safe and trouble-free operation of the unit:

Equipotential bonding conductor



In addition to the protective earth conductor of the mains power cable, the equipotential bonding conductor (section 5.1, No. 22) a direct connection between the electrical unit and the equipotential bonding rail of the electrical system. This reduces the risk of housing leakage currents becoming too high.

- Connect the equipotential bonding cable to the equipotential bonding connection and the equipotential bonding rail. Make sure that a properly functioning and suitable equipotential bonding conductor and equipotential bonding cable are used (e.g. according to DIN 42801).
- Before connecting the unit, compare the electrical data (voltage and frequency) on the nameplate to the electrical data of your mains power supply. This data must match to prevent the unit from being damaged. When in doubt, please ask your electrician for advice.
- The electrical power outlet must be protected by a 16A circuit breaker.
- Use the cable supplied with the unit to connect the unit to the mains supply. The power cable socket is located on the rear of the unit (see section 5.1, "Views of the unit, control elements, and display elements").
- The power supply at the installation site must meet the requirements for electrical systems in hospitals and medical environments (see VDE 0100-710 "Low-voltage electrical installations Part 7-710: Requirements for special installations or locations - Medical locations.").

5 Design and function

This chapter contains important information about the design and function of the unit.

5.1 Views of the unit, control elements, and display elements

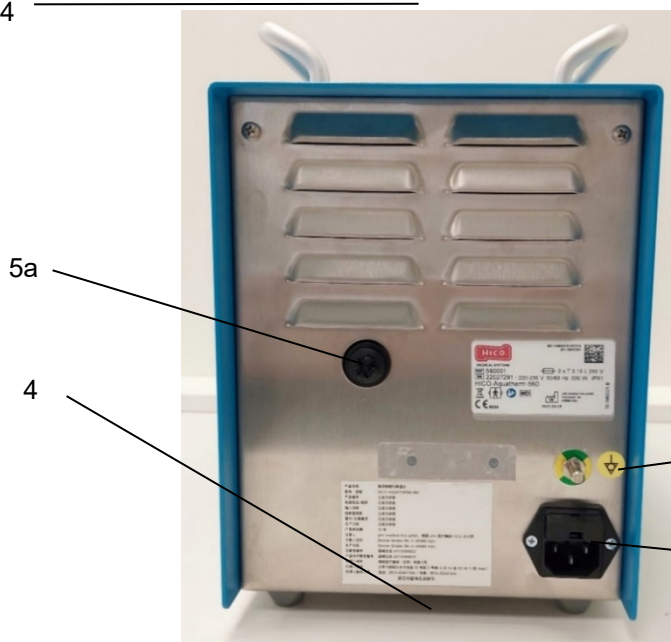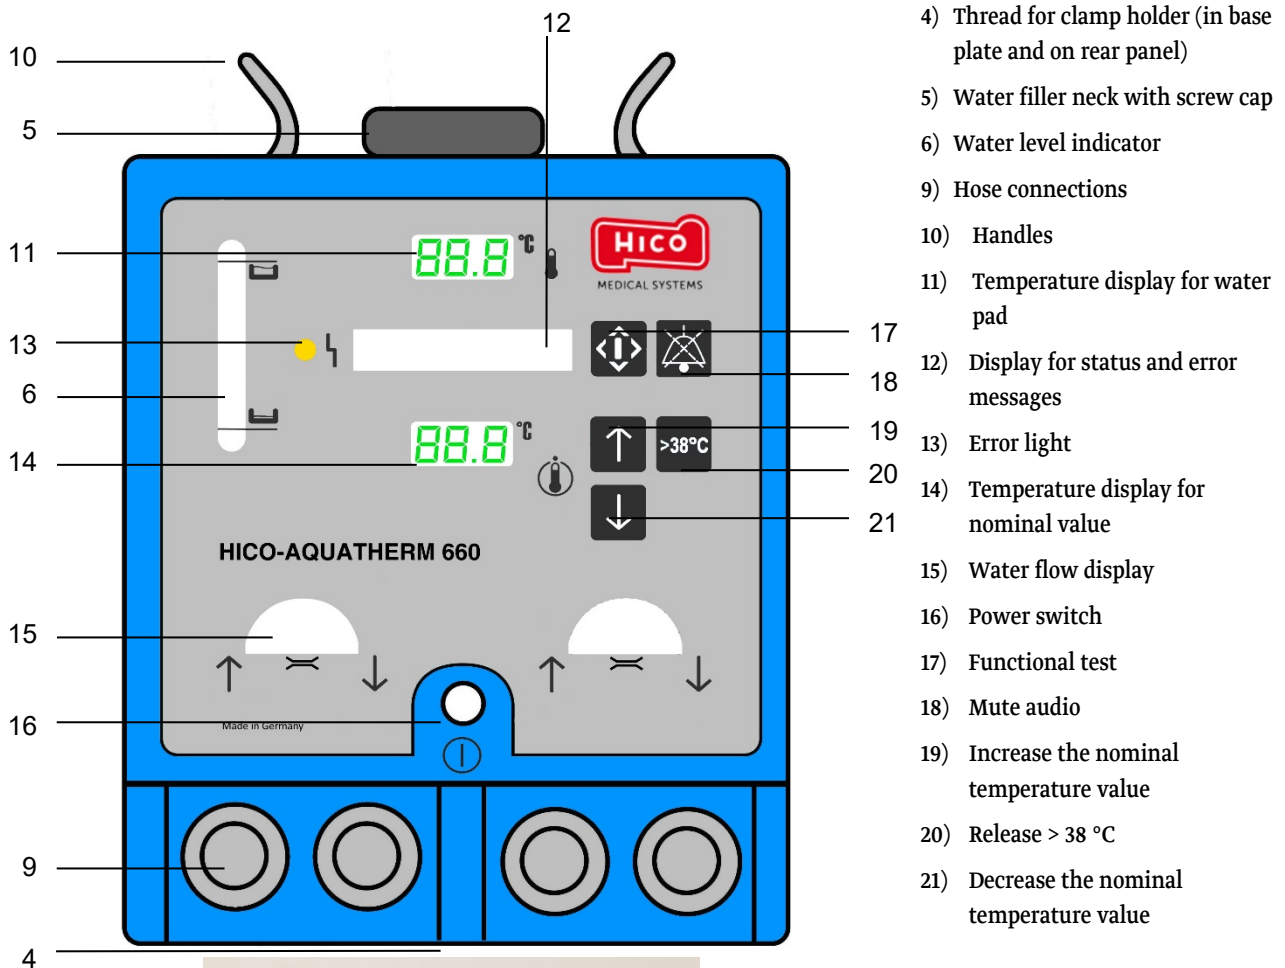

Rear view of the unit:

5a) Water drain outlet with screw cap

22) Equipotential bonding bolt with colour marking and label

23) Microfuse and power cable socket

5.2 Safety devices

5.2.1 Sensors

During operation, the HICO-AQUATHERM 660 monitors

- the water level in the unit,
- if the water temperature in the circuit matches the nominal temperature value set,
- if the unit is connected to power,
- If the unit is functionally safe and emits alarms in case of malfunctions (see section 6.3).

The unit is equipped with an autonomous safety device that prevents the water from dropping below a critical temperature of 3 °C or exceeding 41.5 °C. The result is a maximum surface temperature on the pad that is below 41 °C.

















▲ WARNING

The HICO-AQUATHERM 660 does not have a function for monitoring the patient's measured values.

- ▶ The core temperature of the patient to be treated must be monitored regularly independent of the application system.
- ▶ The temperature settings for the transition temperatures on the pads must be entered manually in the system by the user, and the individual course of therapy should be corrected or adjusted accordingly.

The system should only be used/put into operation by users who are qualified to use the system properly!

5.3 Symbols

	Item number		Serial number
	Manufacturer and country of manufacture: pfm medical hico gmbh Wankelstraße 60 50996 Köln Germany		Also involved in the conformity assessment procedures: SGS Fimko ltd, Takomotie 8 FI-00380 Helsinki Finland
	Medical product		Observe / follow the instructions for use
	Marking of electrical and electronic equipment according to Article 11(2) of Directive 2002/96/EC (WEEE).		The level of protection against electrical shock in the pads corresponds to type BF protection (defibrillation protection).
	2 unit fuses: T: Slow acting fuse, L: Glass fuse, 3.15: Trigger current in A, 250 V: Operating voltage		AC voltage, the unit is only suitable for operation with an AC voltage.
IPX1	Protection against water that drips down vertically (drip water)	V	Rated voltage in volts.
Hz	Rated frequency in hertz.	W	Rated current in watts.
	Equipotential bonding: Marks the connection for the equipotential bonding cable.		LOT number
	Keep away from sharp objects.		Keep out of direct sunlight.
	Temperature limits to which the medical product can be safely exposed.		Caution: Indicates that caution must be taken when handling the unit in the area near the symbol.

5.4Function

5.4.1 Basic principles

The HICO-AQUATHERM 660 hyperthermia unit serves the purpose of warming patients using water pads. The latest safety and application-related knowledge about water pad systems was applied during the development of the unit.

Heat is transferred between the patient and the water pad solely through surface contact. Thanks to its high heat capacity and heat conductivity, water is an ideal transmission medium for this type of application.

The sterile filtered tap water is heated to a temperature of 39 °C in a water tank inside the unit by a heating element and is pumped continuously through the water pad by a centrifugal pump.

The transition temperature to be reached on the pad depends on the environmental conditions and the size of the pad.

The HICO-AQUATHERM 660 is characterised by its safe and easy use, reliability, and compact design.

Using its electronic control, the heat transferred to the patient can be adjusted reliably while simultaneously maintaining high operational safety.

The transition temperature on the patient when warming normally should not exceed 40 °C to prevent the risk of burning when used for a long period of time. This not only a risk when the transition temperature is too high, but also when it is too low. To minimise this risk in case of an equipment failure while warming a patient, the HICO-AQUATHERM 660 switches off electronically and electrically when a water temperature higher than 41.5 °C is reached.

Transition temperatures $> 38\text{ °C}$ must be consciously set by the user and closely monitored.

This virtually rules out the risk of local accumulations of heat, whereby the requirements for the installation site and the site of use also must be fulfilled.

Performance limitations in terms of the attainable pad transition temperatures under extreme ambient conditions or due to the combination of pads selected (see section 6.2.8 “Schematic performance charts”) may also lead to restrictions in the scope its intended purpose.

▲ WARNING

Risk due to overestimation or underestimation of the performance of the system!

Using the unit can also be hazardous when used for its intended purpose if the desired temperatures cannot be reached due to the ambient conditions.

The reliable therapeutic use of the system requires the user to weigh the risks carefully and continuously monitor and care for the patient.

5.4.2 Indications / contraindications / side effects

Indications

In general, the HICO-AQUATHERM 660 can be used in hyperthermia treatment for the following purposes:

- Heat supply in case of intraoperative or postoperative hypothermia
- Heat supply to stabilize the patient's temperature (normothermia)
- Heat supply in case of accidental hypothermia

Contraindications

- Advanced malign disease
- Persistent state of shock / cardiopulmonary instability
- Pregnancy
- Coma of different origin
- Application distal of arterial cross-clamping

▲ WARNING

Risk due to overestimation or underestimation of the performance of the system!

Using the unit can also be hazardous when used for its intended purpose in the following cases:

- ▶ Improper understanding of physical interactions among external accessories and due to ambient conditions (pad size, ambient temperature, etc.)
- ▶ Individual and unpredictable patient reactions

The reliable therapeutic use of the system requires the user to weigh the risks carefully and continuously monitor and care for the patient.

Side effects

The materials used in water pad systems have no known side effects.

In applications, the transfer of heat using water pads may be considered unsatisfactory if the following is true:

- Less than 20 % of the surface of the water pad comes into contact with the patient.
- The contact pressure reduces skin circulation. In this case there is an additional risk of bedsores.

In warming applications and the corresponding specific increase of the patient's temperature, there is always a risk of burning during long-term applications and when the temperature is too high.

In case of a heat loss and the associated unintentional reduction of the patient's temperature (hypothermia), the following side effects can occur:

- Autonomous reactions (among others, shivering)
- Electrolyte imbalances
- Excess urination (diuresis fluctuations)
- Hyperglycaemia (glycaemic fluctuations)
- Greater blood loss (due to reduced blood-clotting factors)
- Changes in the pharmacokinetics
- Higher wound infection rates (sepsis)
- Risk of decubitus

▲ WARNING

Uncontrolled hypo/hyperthermia associated with increased patient mortality.

- ▶ If the body temperature falls below 32 °C, then life-threatening complications may occur such as cardiac arrhythmia, metabolic disturbances, and cardiac arrest.
- ▶ After hypothermia treatment, the temperature of the patient should be increased by no more than 0.25-0.5 °C per hour. Warming too rapidly also leads to arrhythmias and ventricular fibrillation with the subsequent risks.
- ▶ When used on ischaemic limbs, there is an increased risk of tissue damage and shock.
- ▶ Applying additional heat when administering transdermal medications can increase the delivery of the transdermal medication and damage the health of the patient.

▲ CAUTION

- ▶ For the low-risk and reliable application of hypo/hyperthermia treatment, it is of utmost importance to externally and continuously monitor the body core temperature (e.g. by measuring the temperature in the urinary bladder).
- ▶ Mild to moderate therapeutic hypothermia requires the user to weigh the risks carefully and continuously monitor and care for the patient to detect side effects, prevent pressure-induced lesions, and ensure the efficiency of the system.
- ▶ Only leave the water pad in contact with the patient during normal operation. Due to the excellent heat conductivity of water, the patient may cool down when the unit is switched off or the water pad is disconnected from the unit.
- ▶ No distal application of an arterial clamp!

NOTE

The medical information provided here does not claim to be current or complete since new discoveries are constantly being made in the field of hypo/hyperthermia.

The pfm medical hico gmbh is not responsible or liable in any way for negligent or incorrect use and cannot provide any medical recommendations or procedures.

6 Control and operation

This chapter contains important instructions and information for operating the unit. Please follow these instructions to avoid danger and prevent damage.

6.1 Before switching on

6.1.1 Check the unit

Inspect the unit for external damage.

Check the water level before and after

- switching on the unit and
- connecting a water pad.

The water level must be between both marks on the water level indicator (6), preferably just below the maximum mark. The difference in volume between the two marks is approx. 1.0 litre.

Fill with sterile filtered tap water to which a disinfectant has been added when the following applies:

- The water level is below the minimum mark.
- You want to connect an empty water pad and the water level is below the maximum mark.

6.1.2 Water pads

- Only connect original HICO hose extensions with HICO water pads or HICO qualified water pads to the HICO-AQUATHERM 660.
- Check the water pads for external damage before connecting. Use only undamaged pads.
- Have a collecting basin ready in case a pad should start leaking.
- Place a thin fleece between the water pad and the patient's skin.

Water pads can be connected and disconnected regardless of whether the unit is switched on or off.

NOTE

Disconnecting water pads when the unit is switched on and in heating mode:

- ▶ Reduce the nominal temperature before disconnecting the water pad. Otherwise the sterile filtered tap water in the unit's circuit can briefly rise more than 1 °C above the temperature setting or exceed the upper temperature limit, and the unit may trigger various alarms.

NOTE

Intermediate layers between the patient and water pad (bed sheets, surgical drapes, gel pads, etc.) adversely affect the heat transfer.

- ▶ A thin, absorbent cotton or fleece cloth must be placed between the water pad and the patient's skin. Direct skin contact with the pad, which is made of plastic, can lead to skin damage and increases the risk of decubitus.
- ▶ Make sure there are no creases in the fleece after placement.

6.1.3 Heat output

Information: During operation the display on the unit shows the amount of heat transferred (heat output) by the unit to the heating pad, which means it shows the heat output in Watt (W) that was transferred to the environment (air, contact surfaces of the operating table, etc.) and to the patient.

The percentage of the amount of heat displayed that is actually transferred to the patient depends on the type and size of the heating pad and is always less than 100 %.

The better the heating pad is thermally insulated from the underlying surface (e.g. the operating table) and the higher the ratio of the contact area with the patient to the total area of the heating pad, the higher the percentage of the total heat output that is transferred to the patient.

6.2 Operation

6.2.1 Switching on for the first time



- Switch the unit on using the power switch (16); when switched off, the power switch is flush with the front panel.
- If the temperature setting is higher than 38 °C, then check if the temperature setting is actually correct before pressing the release key (20).
- Run the unit for about two minutes to remove any air from the circuit in the unit.
- Check the water level on the indicator (6); if necessary, switch off the unit using the power switch (16), disconnect the power cable from the mains supply, and refill it with sterile filtered tap water to which a disinfectant has been added.
- Connect a water pad to the unit; the pad and the unit should be at the same level.
- Reconnect the unit to the mains supply, switch it on, and run it for another two minutes to force all the air out of the water pad.
- Check the water level again on the indicator (6); if necessary, switch off the unit using the power switch (16), disconnect the power cable from the mains supply, and refill it with sterile filtered tap water to which a disinfectant has been added.
- Repeat the procedure when connecting a second pad.
- After use, switch the unit off using the power switch (16) and disconnect the power cable from the mains supply.

6.2.2 Switching on in normal operation



- Switch the unit on using the power switch (16); when switched off, the power switch is flush with the front panel.
- If the temperature setting is higher than 38 °C, then check if the temperature setting is actually correct before pressing the release key (20).
- Check the water level on the indicator (6), especially if you have connected an empty water pad.
- After use, switch the unit off using the power switch (16) and disconnect the power cable from the mains supply.

6.2.3 Functional test

After switching the unit on, it automatically performs a function test. During this test, monitor the displays to ensure they behave as described in the following:

- A short audible alarm indicates that the unit is ready in case of a power failure alarm.

The unit now checks its autonomous safety device and does the following:

- Shows the result in the display (12)
- The temperature displays (11) and (14) show **88.8**
- The yellow error light (13) lights up
- The audible alarm is triggered.

This test takes a few seconds.

▲ CAUTION

If the unit does not pass all functional tests successfully, then the unit is no longer safe to operate.

Do not operate unit in the following cases:

- ▶ The unit does not sound the short signal tone for the power failure alarm when switching on.
- ▶ The alarm sounds continuously.
- ▶ The automatic function test automatically switches the unit off because it has detected a defect in the independent safety device.
- ▶ The display has failed.
- ▶ Individual segments of the temperature display have failed (temperature can no longer be read properly).
- ▶ The yellow error light (13) is continuously lit or does not light up at all (functional test).
- ▶ The unit does not respond when you press a key.

In these cases, have the unit to be checked by HICO Customer Service.

6.2.4 Setting the temperature



- Set the nominal value for the water temperature - i.e. the temperature on the contact area between water pad and patient - using the two arrow keys (19) and (21). The temperature can be adjusted in increments of 0.1 °C between 35 °C and 39 °C. The temperature display (14) shows the nominal temperature setting.

For temperature settings above 38 °C, press the up arrow key (19) and the release key (20) at the same time.

▲WARNING

- ▶ At temperatures below 35 °C, heat is withdrawn from the patient at a higher rate.
- ▶ At temperatures over 38 °C, the patient is provided with heat at a higher rate.
- ▶ Regardless of the temperature, parts of the body that are subjected to increased pressure may suffer from pressure necrosis and/or burns. This applies especially to long-term applications and high-risk patients.⁶

▲CAUTION

To ensure reliable indications and safe operation, note the information in sections 4.2.1, 5.4.2, 6.2.8, and 6.2.9!

External conditions and pad size influence the nominal temperature setting, e.g. very high or low temperature settings may not be reached under some circumstances in environments with high or low ambient temperatures and/or when connecting one large pad or two smaller water pads. In this case, set the temperature to a lower or higher value until the unit can reliably regulate the temperature.

⁶ Cf. Scott S.M., Thermal blankets injury in the operating room, Arch. Surg. 34, page 181, 1967

NOTE

The unit does not actively regulate the temperature to a temperature setting that is lower than the current temperature value. The water pad is cooled passively according to the ambient temperature or by the body temperature of the patient. The message “TEMP.DIFF. > 1°C”, “ACTIVE COOLING”, “NOT POSSIBLE”.

Heat transfer:

Heat is only transferred (supplied) between the patient and the water pad if the temperature of the water pad is higher than the skin temperature of the patient on the contact surface.

The rate of heat transfer is directly proportional to the following:

- The difference between the skin temperature and the water pad temperature
- The size of the contact area

Intermediate layers impair heat transfer (e.g. surgical drapes or gel pads).

Example of a temperature difference:

The heat transfer from the pad to the patient doubles when the temperature difference between the water pad and the patient is doubled. If the patient's skin has a temperature of 34 °C on the contact area and the water pad temperature is raised from 36 °C to 38 °C, then the heat transfer will double because the temperature difference is doubled from 2 °C to 4 °C.

Due to the thermoregulation of the patient, this is only an approximation.

Example of enlarging the contact area:

To enlarge the contact area, you can connect two water pads of the same type or of different types to the unit.

With a larger contact area, more heat is transferred, even when the temperature difference is smaller. The pad temperature - i.e. the nominal temperature value - can be set to a value that is closer to the patient's temperature.

6.2.5 Temperature control mode

▲WARNING

There is a risk of the patient becoming overheated or undercooled.

- ▶ The patient's body temperature must be monitored when using the unit and water pad on the patient.

If the nominal temperature is set to a value between 35 °C and 38 °C, then the unit will start normal operation automatically after it is switched on and after the function test, and will maintain the water temperature in the water circuit of the system at the temperature setting.

If the nominal temperature is set to a value higher than 38 °C, then the unit will emit an audible alarm, and the message "NOMINAL VALUE >38°C!", "RELEASE KEY" will appear in the display (12).



Check if the nominal temperature setting is correct, and only press the release key (20) if it is correct.

The unit starts the temperature control mode and shows "HEATING ACTIVE" in the display (12) when the temperature setting is higher than the actual temperature.

The unit does not actively regulate the temperature to a temperature setting that is lower than the current temperature value.

▲CAUTION

Only leave the water pad in contact with the patient during normal operation.

Due to the excellent heat conductivity of water, the patient may cool down when the unit is switched off or the water pad is disconnected from the unit.

NOTE

If a nominal temperature is not reached within 30 minutes after switching on the system due to external conditions and the size of the pad, then an alarm message (TEMP.DIFF >1 °C) will appear (see section 6.3.2 "Alarm descriptions during operation").

6.2.6 Handling water pads**NOTE**

- ▶ Avoid contact with hot, sharp, and pointed objects.
- ▶ When disconnecting a water pad from a unit that is switched off, the pad should be lower than the unit. This prevents backflow, and the pads stay sufficiently filled with sterile filtered tap water for the next use.
- ▶ Water pads connected to the unit should never be stored at a higher level than the unit, e.g. never on top of the unit. Otherwise the sterile filtered tap water will flow from the pad back into the unit and overflow.
- ▶ Water pads should be stored rolled up whenever possible. Creases and kinks can damage the material.
- ▶ Avoid direct sunlight. Heat and UV rays will damage the material.

6.2.7 Using water pads

The water pads can be placed horizontally and be used both as an underlay underneath the patient and as a cover over the patient. It is also possible to wrap smaller pads around them necessary. It is important to ensure the pad and the hoses are free of creases and kinks after placement so that the water flow is not affected and no unnecessary pressure is applied to the patient. Make sure the contact surface between the pad and the patient is as large as possible given the particular pad size. It is recommended to use a thin fleece as an intermediate layer. Direct skin contact with the pad, which is made of plastic, can lead to skin damage and increases the risk of decubitus. Make sure here as well that there are no creases in the fleece after placement.

External conditions and pad size influence the nominal temperature setting that can be reached, e.g. very high or low temperature settings may not be reached under some circumstances when connecting one large pad or two smaller water pads. After starting the unit, monitor the nominal and actual temperature differences and, after approx. 45-40 min of operation, set the temperature on the unit to a lower or higher nominal value that approximately corresponds to the actual value.

NOTE

- ▶ For trouble-free and stable operation, the difference between the nominal temperature setting and actual temperature displayed on the unit should not be greater than 1 °C.
- ▶ The thicker the intermediate layers between patient and water pad are (bed sheets, surgical drapes, gel pads, etc.), the poorer the heat transfer.

6.2.8 Schematic performance charts

Explanation:

The data for the performance diagrams was obtained in an appropriate setting in the laboratory at three different ambient temperatures and for three different pad combinations.

Desired pad temperatures: 39 °C⁷

Ambient temperature: 10 °C, 20 °C, and 30 °C

Water temperature at start of test: 20 °C

Pads used:

1 smallest pad: L x W: (50 x 30) cm / area: 1,500 cm²

2 largest pad: L x W: (170 x 50) cm / area: 8,500 cm²

The pad sizes selected are representative of other HICO pad sizes used in applications.

The following performance charts illustrate limit value analyses (at extreme conditions) for ambient temperatures, pads, and settings based on data obtained according to standard laboratory procedures.

This leads to the following restrictions:

- No restrictions

The values shown the performance charts are approximate values.

⁷ In accordance with the requirements of IEC 60601-2-35, the temperature of the system is limited to 39 °C.

Performance charts:


The temperature limit values⁸ to be reached within 10 minutes to 60 minutes (see diagrams 1-3) after startup and adjustment of the temperature setting during operation under laboratory test conditions.

▲ CAUTION

In actual applications, the temperature limit values may differ!!


When used in actual applications, follow the instructions and note the warnings and information, etc., from the relevant sections:

- 4.2.1 Requirements on the installation site / operating location
- 5.4.1 Basic principles
- 5.4.2 Indications / contraindications / side effects
- 6.2.5 Temperature control mode
- 6.2.7 Using water pads
- 6.2.8 Schematic performance charts
- 6.2.9 Responsibilities during operation
- 6.3.2.2 Alarms; *Display message: TEMP.DIFF > 1°C*

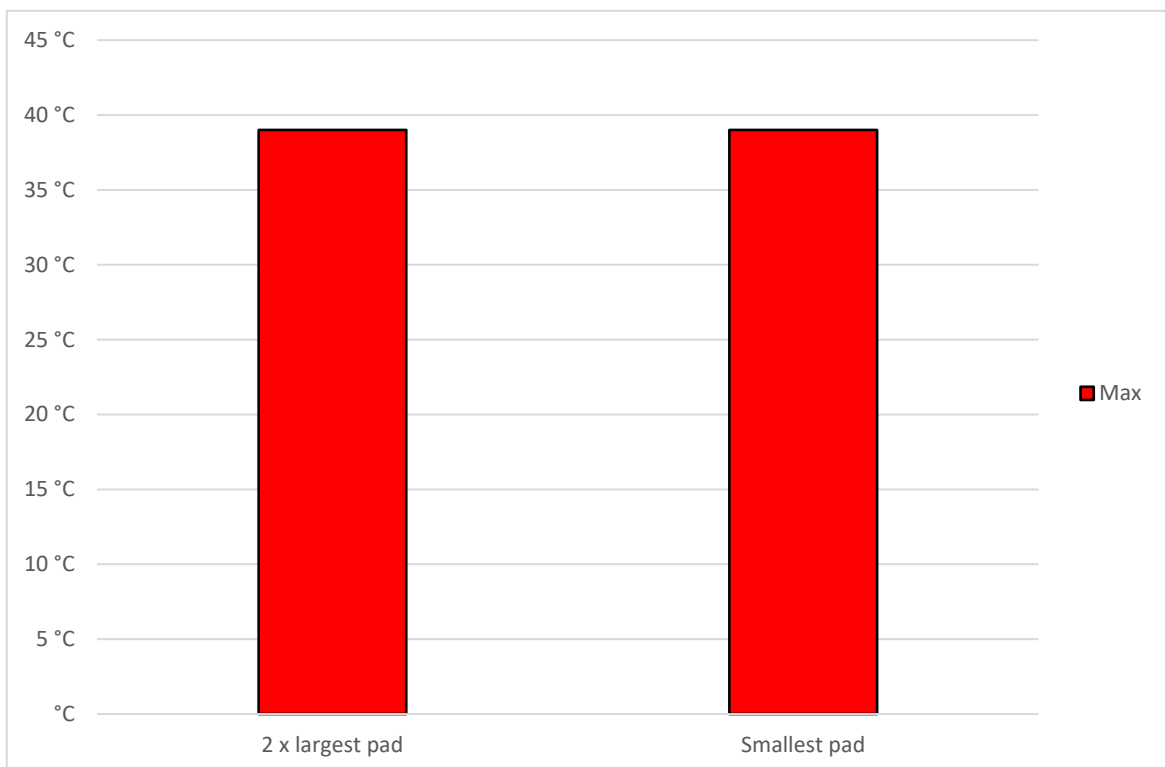


Performance Chart 1 - Ambient Temperature 10 °C

⁸ The temperatures shown are reference values from the schematic performance charts of the laboratory analyses. They do not claim to be completely accurate when actually using the system.

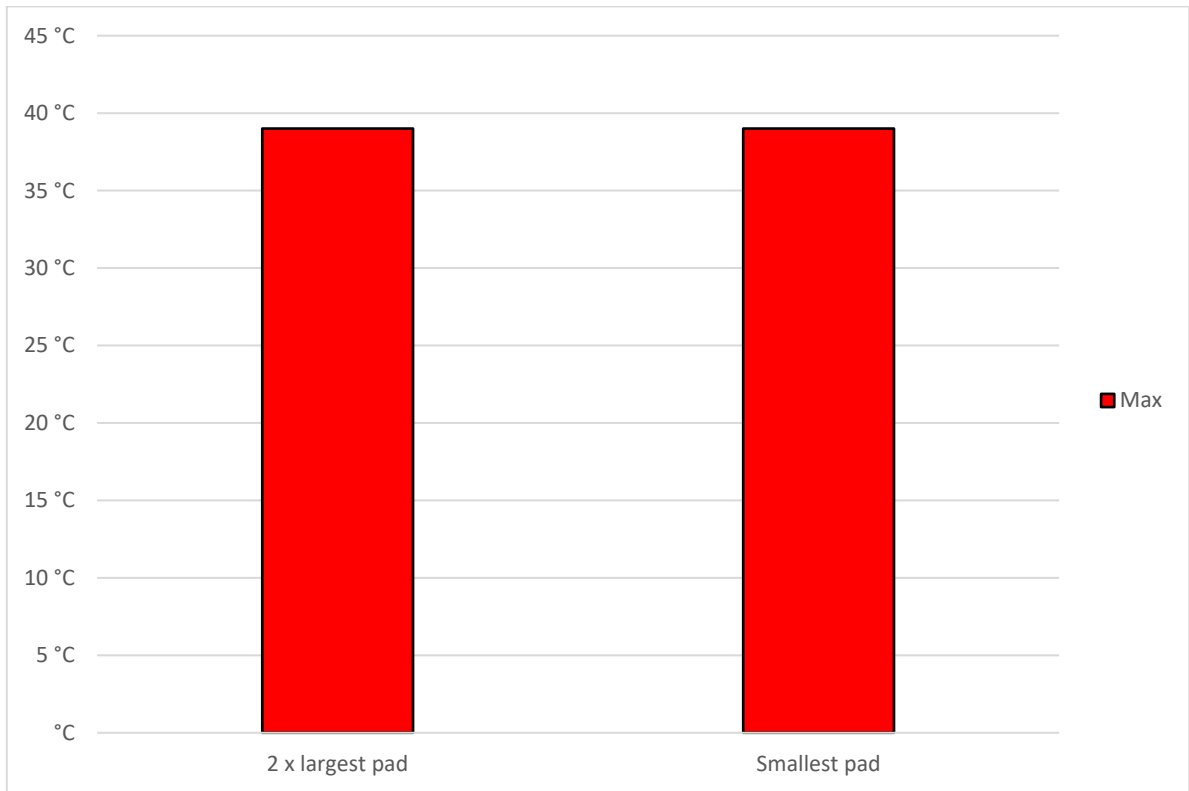

Performance Chart 2 - Ambient Temperature 20 °C

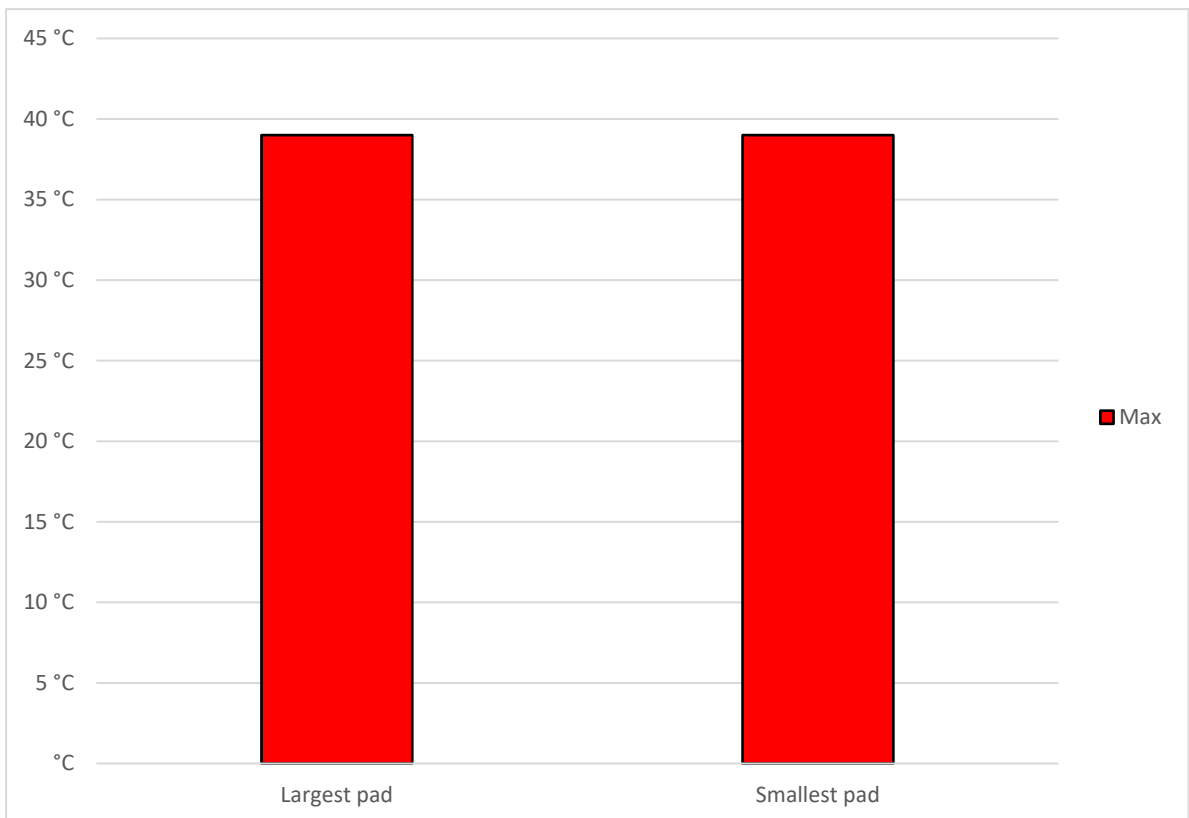

Performance Chart 3 - Ambient Temperature 30 °C

6.2.9 Responsibilities during operation

6.2.9.1 Indication-based

▲ WARNING

Risk due to overestimation or underestimation of the performance of the system!

Using the unit can also be hazardous when used for its intended purpose in the following cases:

- ▶ Improper understanding of physical interactions among external accessories and due to ambient conditions (pad size, ambient temperature, etc.).
- ▶ Individual and unpredictable patient reactions.

The reliable therapeutic application of the system requires the user to carefully weigh the risks between the desired indication and the performance of the system, as well as to continuously monitor and care for the patient in terms of side effects and preventing the formation of pressure ulcers due to heat or cold.

For the low-risk application of hypo/hyperthermia treatment, it is of utmost importance to externally and continuously monitor the body core temperature, e.g. by measuring the temperature in the urinary bladder, because uncontrolled hypo/hyperthermia is associated with increased patient mortality. See section 5.4.2 for indications / side effects / contraindications.

NOTE

The medical information provided here does not claim to be current or complete since new discoveries are constantly being made in the field of hypo/hyperthermia. The pfm medical hico gmbh is not responsible or liable in any way for negligent or incorrect use and cannot provide any medical recommendations or procedures. The user must independently decide what to use and how to proceed.

6.2.9.2 System-based

Check the water flow

During operation, check the water flow in the unit and the pad at regular intervals. The sight glass of the water flow indicator (15) features an impeller. When the flow of water is optimal, it is impossible to focus on the individual blades of the impeller.



Performing a function test

During long-term operation, check the independent safety device manually at least once every day. For this purpose, press the function test key (17) during operation. The unit then tests the safety electronics:

- The alarm sounds
- The temperature displays show **88.8**
- The yellow error light (13) lights up
- The display shows FUNCTION TEST.

After passing the test, the display shows the message “FUNCTION TEST OK”, and the unit automatically resumes normal operation.

▲ CAUTION

If the function test was not completed successfully, then the unit is no longer safe to operate. In this case;

- ▶ Do not use the unit on a patient.
- ▶ Have the unit inspected by Customer Service.

Checking the temperature control mode

During long-term operation, check the nominal temperature setting and actual temperature values shown in the display regularly; see section 6.2.5 and 6.3.2.

6.2.10 Operating language

The status and error messages in the display (12) can be displayed in the following languages: German, English, French, Spanish, Italian, and Polish. Set the display language as follows:



- Switch the unit on.
- Hold the “Audio paused” (18) key down for about 4 seconds; the last language setting used appears in the display.
- Keep pressing the “Nominal value higher” (19) arrow key until the desired language appears in the display.
- About 10 seconds after the last input, the unit will return to its previous operating status, and the last language displayed is the active language.

6.3 Alarms

6.3.1 General information

In the event of an alarm, the unit always emits both visual and audible alarm. The operator is therefore notified immediately in case of a malfunction, which increases the operational reliability of the system. The display (12) shows the error that caused the alarm (except in the case of a power failure alarm).

The alarms are assigned a medium priority⁹. Ignoring an alarm can result in the following:

- Minor injuries or discomfort within a period of time that is usually not long enough for manual corrective action (immediately).
- Reversible injuries within a period of time that is usually long enough for manual corrective action (promptly).
- Death or irreversible injury within an undefined period of time that is greater than the “promptly” time period (delayed).

If the system sounds an alarm for the reasons described in section 6.3.2, then the alarm can be reset as follows depending on the expected result.



- Pressing the “Mute audio” key (18) interrupts the audible alarm for 10 minutes. The error message can be read in the display (12). The error light (5) continues to flash as long as the alarm condition is present. The alarm condition must be eliminated according to the alarm message shown on the display (12).
- The unit switches all functions off. The audible alarm cannot be interrupted. Switch off the unit using the power switch (16), take it out of service, and if necessary, have it inspected by a service technician (Customer Service / Medical Technology).

NOTE

Before pressing the “Mute audio” key (18) or the power switch (16) to suppress the alarm or take the unit out of service, please read the error message in the display!

6.3.2 Description of alarms during operation

6.3.2.1 *Display message: WATER LEVEL!?*

The unit triggers this alarm when the water level drops below the MIN mark on the water level indicator (6) during operation. The display shows

⁹ Source: IEC 60601-1-8 Table 1 - Alarm condition priorities

“WATER LEVEL!?” , the yellow error light (13) flashes, and a pulsating signal tone sounds.



- Press the “Mute audio” key (18) to interrupt the audible alarm for 10 minutes.
- Immediately fill up sterile filtered tap water to which a disinfectant has been added, until the water level is just below the MAX mark (6) (see section 4.3.1 “Filling the system”).

▲ CAUTION

- ▶ When the water level is too low, adequate water circulation can no longer be guaranteed.
- ▶ A water level that is too low can cause damage to components of the unit and consequently lead to the total failure of the unit.

6.3.2.2 Display message: TEMP.DIFF > 1°C

If the temperature of the water pad deviates from the temperature setting by more than 1 °C during operation, then the unit will trigger this alarm. The display shows “TEMP.DIFF. > 1°C”, the yellow error light (13) flashes, and a pulsating signal tone sounds.



- Press the “Mute audio” key (18) to interrupt the audible alarm for 10 minutes.
- Change the temperature setting until the unit is able to regulate the temperature reliably.

NOTE

- ▶ Connecting or disconnecting a water pad during operation can create a temperature difference that causes the alarm to trigger.
- ▶ The alarm can be triggered due to unfavourable room temperatures and/or when large pads or two water pads are connected because the specified nominal temperature (e.g. 39 °C) cannot be reached in this case. Change the temperature setting until the unit is able to regulate the temperature reliably.
- ▶ After switching on the unit and changing the temperature setting, this alarm function is suppressed for a defined period of time.

6.3.2.5

Display message: CHECK UNIT →CUSTOMER SERVICE

The unit triggers this alarm in case of various defects. The display shows “CHECK UNIT” and “CUSTOMER SERVICE”, the yellow error light lamp (13) flashes, and a pulsating signal tone sounds.

The audible alarm **cannot** be interrupted using the “Mute audio” key (18).

- Switch off the unit using the power switch (16).

Take the unit out of service and have it inspected by a service technician (Customer Service / Medical Technology). The number displayed after “CHECK UNIT” is intended as information for service technicians. (Customer Service / Medical Technology).

6.3.2.6

Power failure alarm

The unit triggers this alarm when the mains power supply fails during operation. The yellow error light (13) is lit and a signal tone sounds. All other displays have no function. The power accumulator in the unit can maintain the alarm for at least 120 seconds in the event of a power failure.

The audible alarm **cannot** be interrupted using the “Mute audio” key (18).

- Switch off the unit using the power switch (16).

NOTE

The alarm automatically turns off when the mains power supply returns.

The last temperature setting is stored in the unit.

When power is restored, the temperature setting stored must be checked by the user and confirmed before the unit returns to normal operation (see section 6.2 “Operation”).

6.3.2.7 Software-related alarm messages

The unit can display alarm messages for various software-related errors. The message “POST ERROR” is then displayed followed by a number as well as one of the following additional messages “POST ERR CRC”, “POST ERR WD”, “POST ERR RTC”, “POST ERR VOLT”, “POST ERR EEPROM”, or “ERR SYSTEM PARAM” “ERROR” followed by a number.

The messages “SUPER STATE NOT ACTIVE” or “FATAL ERROR SYSTEM HALT” can also be displayed.

The source of these error messages may be a software malfunction.

- Switch off the unit using the power switch (16) and have it inspected by a service technician (Customer Service / Medical Technology).

7 Cleaning and disinfection

This chapter contains important information on cleaning and disinfecting the unit. Please follow these instructions to avoid damage to the unit due to improper cleaning and to ensure trouble-free operation.

7.1 Safety instructions

▲ CAUTION

Follow the safety instructions below before starting to clean the unit.

- ▶ Disconnect the power cable before you start cleaning and disinfecting the unit.
- ▶ Do not allow any fluids to get inside the unit.
- ▶ Do not use any spray disinfectants on the unit.
- ▶ Let the unit dry completely before switching it on again.

▲ CAUTION

Sensitive surfaces

The surfaces of the unit and the pads can be destroyed when you use the wrong cleaning agents and disinfectants.

- ▶ Use only disinfectants based on aldehydes, ammonium compounds, or alcohols that do not affect ABS plastics, PVC, or PU on all surfaces and parts.
- ▶ Do not use any disinfectants based on phenol derivatives because these will shorten the lifespan of plastic materials.

7.2 Unit

7.2.1 Water circuit

7.2.1.1. General Information for cleaning the water circuit

The cleaning process consists of a total of three steps. Thoroughly clean the unit (basic cleaning) and the accessories first, then disinfect the unit, and then flush and refill the unit. The cleaning process must be performed once a month. You must wear disposable gloves during the entire cleaning process and avoid contact with the sterile filtered tap water and the disinfectant.

7.2.1.2. Basic cleaning

Disconnect the unit from the mains power supply and remove any accessories that may be connected to it. Completely empty the unit and all accessories (e.g. water pads, extension hoses, etc.). Refill the unit with a neutral cleaner (follow the manufacturer's instructions) and use only sterile filtered tap water to dilute the cleaner. Connect the parts and accessories to be cleaned to the unit and connect the unit to the mains power supply. Use the arrow buttons to set the temperature to 35 °C. Turn on the unit and leave it on for 30 minutes. Disconnect the unit from the mains power supply and remove the connected parts and accessories. Completely empty the unit and all accessories.

7.2.1.3. Disinfection

For disinfection purposes, the VAH¹⁰-listed disinfectant Sanosil S003, which is free of phenolic derivatives, can be used.

Note the dosage recommended by the manufacturer of the disinfectant. If necessary, prepare a disinfectant solution according to the instructions of the manufacturer of the disinfectant. Fill the unit with the disinfectant or the disinfectant solution. Connect the device to the mains power supply and connect all parts and accessories to be disinfected to the unit. Switch on the unit and allow it to run for about two minutes so that the disinfectant can be distributed throughout the circuit; if necessary, add more disinfectant or disinfectant solution. Switch off the unit and note the exposure time specified by the manufacturer of the disinfectant. After the exposure time has expired, disconnect the unit from the mains power supply and completely empty the unit and all accessories.

▲ CAUTION

¹⁰German Association for Applied Hygiene (Verband für Angewandte Hygiene), and the list is available from the mhp-Verlag, Wiesbaden

Do not apply any cleaning and decontamination methods other than the ones recommended by pfm medical hico gmbh.

Before introducing new methods, have them checked together with pfm medical hico gmbh.

This is the only way to make sure that the unit will not be damaged by the new method.

7.2.1.4. Flushing and refilling

Fill the unit with sterile filtered tap water¹¹. Connect the unit to the power supply. Connect any accessories you want to use to the unit. Switch on the unit and allow the water to circulate for five minutes. Disconnect the unit from the power supply. Completely empty the unit and all accessories used. The cleaning process is now finished. Before putting the unit back into service, refill the unit using only sterile filtered tap water to which a disinfectant has been added¹².

7.2.2 Surfaces

If possible, use decalcified water to clean the surfaces of the unit. Only wipe the unit with a damp cloth. Use only warm water (max. 50 °C) to which a mild commercial dishwashing liquid has been added. Wipe off again with clean water and wipe the unit dry with a cloth.

To disinfect the surfaces of the unit, we recommend using a wipe-down or surface disinfectant from the VAH list¹³ (e.g. Mikrozid AF from S&M). When using a disinfectant, follow the instructions of the manufacturer.

Only switch on the unit after the disinfectant has evaporated completely.

7.2.3 Ventilation slots

Check the ventilation slots on the back of the unit for dirt and dust regularly (at least every 6 months). Remove as much dirt and dust from the surface as possible. Dust deposits in the unit reduce the performance of the system.

¹¹ Depending on the quality of the water (e.g. its hardness, among other things), the lifetime of the parts of the unit that come into contact with water may be reduced.

¹² For example 10 ml SANOSIL mixture (from Sanosil, Farchant) ⇔ (1000 ml sterile filtered tap water + 10 ml Sanosil solution). If you have any questions, please contact the Customer Service department of pfm medical hico gmbh.

The use of a disproportionately high amount of disinfectant can reduce the lifetime of parts of the unit that come into contact with water. The use of too much disinfectant can also immediately cause malfunctions, for example due to the excessive formation of foam!

¹³ German Association for Applied Hygiene (Verband für Angewandte Hygiene), and the list is available from the mhp-Verlag, Wiesbaden

Have dirt and dust inside the unit removed by a service technician (Customer Service, Medical Technology). Do not open the unit yourself.

▲ CAUTION

Do not apply any cleaning and decontamination methods other than the ones recommended by pfm medical hico gmbh.

Before introducing new methods, have them checked together with pfm medical hico gmbh.

This is the only way to make sure that the unit will not be damaged by the new method.

7.3 Water pads, hose extension

If possible, use decalcified water. Wipe off the surfaces with a damp cloth only. Use only warm water (max. 50 °C) to which a mild commercial dishwashing liquid has been added. Wipe off again with clean water and wipe the pad until dry.

To disinfect the surfaces of the unit, we recommend using a wipe-down, surface, or spray disinfectant from the VAH list¹⁴ (e.g. Terralin protect from S&M). When using a disinfectant, follow the instructions of the manufacturer.

Only use the pad again after the disinfectant has evaporated completely. Check the pad for damage, deformation, and cracks; replace the pad if necessary.

▲ CAUTION

Do not apply any cleaning and decontamination methods other than the ones recommended by pfm medical hico gmbh.

Before introducing new methods, have them checked together with pfm medical hico gmbh.

This is the only way to make sure that the unit will not be damaged by the new method.

¹⁴German Association for Applied Hygiene (Verband für Angewandte Hygiene), and the list is available from the mhp-Verlag, Wiesbaden

8 Maintenance and safety check

This chapter contains important information on the maintenance of the unit. Please follow these instructions to avoid damage to the unit caused by inadequate maintenance and to ensure trouble-free operation.

8.1 Maintenance

We recommend closing a maintenance contract with the pfm medical hico gmbh. By closing a maintenance contract, you fulfil the following requirements:

- Ordinance on Industrial Safety and Health of the German Employers' Liability Association (BetrSichV BGV A2, VBG 4) and the new BGV A3
- Regulation (EU) 2017/745 on medical devices (MDR)
- German Medical Devices Operator Ordinance (MPBetreibV)

All of these regulations require regular technical inspection of the units.

Furthermore, maintenance by our experts ensures maximum operational reliability and the longevity of the unit.

NOTE

With proper handling and regular maintenance, the unit has a product lifetime of about 5 years.

Performing maintenance and safety checks at the specified intervals and repairing when necessary can increase the expected service life of the unit.

NOTE

When handled properly, the lifespan of the necessary accessories (water pads and hose extensions) is determined by the natural aging process and wear through the use of the accessory.

8.1.1 Unit

- Check the ventilation slots on the bottom and back of the unit regularly for dirt and dust.
- Dust deposits in the unit reduce the performance of the system. Have dirt and dust inside the unit removed by a service technician (Customer Service, Medical Technology). Do not open the unit yourself.
- Have the Customer Service or Medical Technology departments perform the maintenance and safety checks regularly to ensure the intervals are maintained.

8.1.2 Water tank

Replace the sterile filtered tap water in the water tank at least once a month (described in section 7.2.1) as follows:

- Disconnect the unit from the mains power supply.
- Place a container (bucket, bowl, etc.) below the front of the unit or place the unit over a drain (e.g. the drain of a sink).
- Unscrew the cap from the water filling neck (5), e.g. with a coin.
- Take the water drain hose and place it on one of the front hose connections (9).
- Tilt the unit forward and drain the water through the water drain hose until it is completely empty.
- Remove the water drain hose from the front hose connection and place it aside for now.
- Clean and disinfect the water circuit as described in section 7.2.1.
- Refill the unit with sterile filtered tap water to which a disinfectant has been added as described in section 4.3.1. The max. filling capacity of the unit tank is approx. 1.4 litres.

8.1.3 Hose connections

The seal rings (O-rings) on all hose connections are subject to aging and can become dry and brittle as a result. You should therefore coat the seal rings with a thin film of silicone paste or petroleum jelly every 6 months.

8.2 Safety check

In order to maintain legal conformity and operational reliability according to the Medical Devices Regulation (EU) 2017/745 (Appendix I, section 23.4(k)) and the German Medical Devices Operator Ordinance (MPBetreibV Art. 6(1)), a safety check must be conducted on the unit every 12 months. The operator is solely responsible for ensuring these safety checks are performed. According to the MPBetreibV (section 6(4)(1+3)), this safety check may only be performed by pfm medical hico gmbh or a qualified person. The safety check covers the following points at a minimum:

- Inspection of the device and accessories for external damage, wear, and aging, and checking the legibility of the displays and labels
- Measurement of the PE resistance and the earth leakage current according to the test facility and manufacturer's data
- Check of all functions according to the instructions for use
- Check of all safety functions according to the manufacturer's data
- Check of all sensors according to the manufacturer's data (pfm medical hico gmbh provides a service manual for authorised persons for this purpose).

8.2.1 Standard configuration for the safety check

When sending the unit in for a safety check, please pack the empty unit together with the hose extension in the original packaging.

NOTE

In order to maintain compliance with statutory safety regulations, we recommend closing a technical safety inspection contract with an authorised company to perform the recommended annual safety check.

▲ CAUTION

For heavily soiled units or accessories returned to us for maintenance or repair where there is a suspicion of contamination due to contact with specific pathogens (e.g. MRSA), the system must be disinfected in advance with an appropriate disinfectant and packaged for transport in accordance with the decontamination requirements and material compatibility. Otherwise we reserve the right to reject such units or accessories for safety reasons, or to subject them to additional treatment (chemo-thermal) before performing a technical revision or damage analysis. Any additional costs arising from such measures shall be borne by the customer.

Questions regarding service, maintenance, or safety checks should be addressed directly to:

pfm medical hico gmbh

Wankelstraße 60

50996 Köln

Germany

Tel.: +49 (0)2 21 / 3 76 78-0

Fax: +49 (0)2 21 / 3 76 78-85

Email: hico@pfmmedical.com

9 Troubleshooting

This chapter contains important information on locating errors and troubleshooting. Please follow these instructions to avoid danger and prevent damage.

9.1 Safety instructions

▲ CAUTION

- ▶ Repairs on electric devices may only be carried out by skilled professionals, including personnel trained by the manufacturer.
- ▶ Improper repairs can seriously endanger the user and cause damage to the unit.

NOTE

Opening the unit by unauthorised persons will void all rights to any guarantee and warranty claims.

- ▶ Repairs to the unit may only be performed by the pfm medical hico gmbh or by experts trained and/or authorised by the pfm medical hico gmbh.

9.2 Causes of error and troubleshooting

When certain errors occur, the unit will switch off all functions. Take the unit out of service and submit it to a service technician (Customer Service / Medical Technology) for inspection and to restore its operational reliability.

Error	Possible causes	Possible actions
No water circulation or insufficient water circulation	<ol style="list-style-type: none"> Hoses or pads are kinked/folded Connections are not tight Unit is positioned far below the heating pad Strong foam formation High patient weight Pump worn/defective 	<ol style="list-style-type: none"> Ensure hoses and pads are correctly placed and positioned Insert hose connections firmly into each other Position the unit at the same height as the heating pad or higher Change the water* Position the unit higher than the heating pad Customer service*
Connectors are hard to connect	<ol style="list-style-type: none"> Sealing ring dry and brittle 	<ol style="list-style-type: none"> Grease sealing ring with petroleum jelly, silicone grease, or a similar lubricant
Hose connection drips constantly	<ol style="list-style-type: none"> Exterior, visible sealing ring damaged or missing 	<ol style="list-style-type: none"> Replace sealing ring*
Coupling valve of the unconnected coupler drips constantly	<ol style="list-style-type: none"> Inner sealing ring damaged Inner sealing ring dirty or contaminated 	<ol style="list-style-type: none"> Customer service* Insert and loosen coupling several times, if necessary contact Customer Service
No heat output value displayed. Display message: "HEAT OUTPUT 0 W" or "HEAT-UP PHASE"	<ol style="list-style-type: none"> Temperature difference (nominal/actual) 	<ol style="list-style-type: none"> Heat is only output when the temperatures are the same
Alarm + display message: "ALARM TEST DEFECT" "->CUSTOMER SERVICE"	<ol style="list-style-type: none"> Independent safety device defective Pump defective (electrical) 	<ol style="list-style-type: none"> Customer service*
Alarm + display message "TEMP.DIFF. > 1°C"	<ol style="list-style-type: none"> Connecting or disconnecting the heating pad during operation 	<ol style="list-style-type: none"> Acknowledge alarm with the "Alarm OFF" key
Alarm + display message every 10 min.: "TEMP.DIFF. > 1°C"	<ol style="list-style-type: none"> Cartridge heater or pump defective Strong foam formation in the tank Bypass interrupted Lack of heat output 	<ol style="list-style-type: none"> Customer service* Change the water* Customer service* Do not operate unit continuously (> 1h) without a heating pad*

Error	Possible causes	Possible actions
Alarm + display message: "WATER LEVEL!?" Can be acknowledged for 10 min. using the "Alarm OFF" key	<ol style="list-style-type: none"> 1. Water level too low 2. Unit is not completely horizontal 3. Sensor deviation 	<ol style="list-style-type: none"> 1. Refill with water 2. Position unit horizontally 3. Customer service*
Alarm + display message: "CHECK UNIT" "->CUSTOMER SERVICE"	<ol style="list-style-type: none"> 1. Various defects 2. Water tank empty 3. Sensor break/short circuit T1 4. Sensor short circuit T2 	<ol style="list-style-type: none"> 1. Customer service* 2. Refill with water* 3. Customer service* 4. Customer service*
Alarm + display message: "CHECK UNIT" "UNDERTEMPERATURE"	<ol style="list-style-type: none"> 1. Unit too cold (< 9 °C) 2. Sensor break T2 3. Water tank frozen 	<ol style="list-style-type: none"> 1. Let the unit warm up at room temperature for a while* 2. Customer service* 3. Let the unit defrost*; Examine unit for frost damage (is water flowing out of the unit?) → Customer service
Unit does not function at all and acoustic alarm	<ol style="list-style-type: none"> 1. Mains power failure 2. Mains connector does not make contact 3. Fuse defective 4. Unit defective 	<ol style="list-style-type: none"> 1. Switch off unit until power returns 2. Check the connector on unit and in the socket for correct fit 3. Customer service* 4. Customer service*

* Switch off the unit immediately

10 Disposal of an old unit



Old electric and electronic devices very often contain precious metals and valuable materials. However, they also contain harmful substances that were necessary for their function and safety.

If disposed of as residual waste or handled incorrectly, these substances can be harmful to humans and damage the environment. This device must not be disposed of together with normal industrial or domestic waste!

For all electrical appliances that you have purchased from us or a specialist dealer after 13.08.2005, we provide you with a return option with our disposal partner enretec GmbH and assume the costs of disposal. To order the disposal of the equipment, you have the following options Phone: +49 800 225 526 3 or e-mail: services@enretec.de. We will be happy to advise and inform you by phone: +49 221 37678-0 or e-mail: hico@pfmmedical.com.

Please prepare the device for transport in accordance with the "Important provisions for the return of an old electrical device" (see enretec.de).

You can arrange the transport to enretec GmbH yourself or commission enretec GmbH to organize the transport. The costs for transport and packaging are always borne by the owner or user of the device

- ▶ According to the product responsibility requirements according to Art. 22 of the German Recycling Economy and Waste Management Act (KrW-/AbfG) and Art. 2(1)(8) of the German Electrical and Electronic Equipment Act (ElektroG), the unit **must** be handed over to a corresponding municipal collection point or returned to the manufacturer.

NOTE

- ▶ After use, medical products and accessories could be contaminated. For this reason, the products and their accessories should be handled and disposed of in accordance with recognized medical procedure, and in compliance with the relevant legal regulations and local ordinances. In accordance with the local waste management regulations, the water pad can be disposed of together with domestic waste for incineration.

11 Technical data, unit, and accessories

11.1 Unit

HICO-AQUATHERM 660

Item No. (REF):	590001 (220-230 V) 590020 (110-115 V)
Rated voltage:	220-230 V, 50/60 Hz 110-115 V, 50/60 Hz
Power consumption:	220-230 V, 530 W 110-115 V, 560 W
Current consumption:	220-230 V, approx. 2.3 A 110-115 V, approx. 4.6 A
Nominal temperature range:	35-39 °C
Safety shutdown:	Approx. 3 °C and 41.1-41.5 °C (hardware) Approx. 7.0 °C and 40.8 °C (software)
Correction value:	0.5 °C (Water temperature display)
Sensor element:	2 x NTC 5K
Pump capacity:	Max. 16 l/min., max. 0.34 bar (10 W)
Heating capacity:	500 W (at 27 °C)
Heat-up time without water pad:	Approx. 5-10 min. (20-37 °C)
Fuse rating:	2 x T 3.15 A L 250 V (220 V / 230 V) 2 x T 5 A L 250 V (115 V)
Class/type of protection:	I, BF (defibrillation protection)
IP protection class:	IP X1 (drip proof)
Risk class ((EU) 2017/745):	II b
Power supply	Must comply with VDE 0100 Part 710: "Electrical safety in medical environments".
Ambient temperature:	10-30 °C
Relative humidity:	Approx. 30-70 %
Transport/storage temperature:	3-60 °C
Air pressure:	700-1060 hPa
Tank volume:	Approx. 0.7/1.4 l (min/max)
Permissible height difference:	Max. 1 m (unit/water pad)
Dimensions WxHxD:	Approx. 200 mm x 290 mm x 330 mm
Weight:	Approx. 7 kg (empty)
Noise emission:	Approx. 35 dB(A) (1 m)
Alarm level:	> 55 dB(A) (3 m)
Test basis:	Regulation (EU) 2017/745 on medical devices (MDR), IEC 60601-1, IEC 0601-1-2, IEC 60601-1-6, IEC 60601-1-8, IEC 60601-2-35
Basic UDI-DI:	4042301Z1204AAVT

Subject to technical changes without notice.

▲ WARNING

It is not permitted to make changes to the HICO-Aquatherm 660!

► No modification of this equipment (device and accessories) is allowed.

11.2 Accessories

- Only HICO qualified water pads (required accessory) may be used together with the HICO-AQUATHERM 660.
- The HICO-Aquatherm 660 can be used with HICO-Polyurethane-Waterpad in combination with HICO-Hose extension, as well as HICO-Polyurethane-Waterpad SP in combination with HICO-Hose extension SP.

Available sizes and empty weights, among others:

HICO-Polyurethane-Waterpad	HICO-Polyurethane-waterpad SP	Dimensions // weight
REF: 550044	REF: 550144	50 cm x 30 cm // 0.24 kg
REF: 550046	REF: 550146	170 cm x 50 cm // 0.91 kg
REF: 550047	REF: 550147	92 cm x 50 cm // 0,54 kg
REF: 550048	REF: 550148	170 cm x 35 cm // 0.67 kg
REF: 550049	REF: 550149	92 cm x 35 cm // 0.44 kg
REF: 550025	REF: 550125	70 cm x 60 cm // 0.52 kg
REF: 550026	REF: 550126	120 cm x 70 cm // 0.90 kg
HICO-Hose extension	HICO-Hose extension SP	Dimensions // weight
REF: 550022	REF: 550090	3 m // 0.43 kg
REF: 600022	REF: 600090	2 m // 0,95 kg, thermo insulated

- In addition to the reusable water pads, Soft-Temp® disposable water pads can be used in combination with the HICO-Hose extension (disposable pads).

Soft-Temp® single-use water pad	Dimensions
REF: 550060	152 cm x 61 cm

REF: 550061	76 cm x 61 cm
REF: 550063	51 cm x 36 cm
HICO-Hose extension (disposable pads)	Length
REF: 550069	3 m

- HICO-Water drain hose (optional accessory; only used to empty the unit)
REF: 550076

NOTE

- ▶ The suitability of the PU pads and accessories for the intended use must be decided by the user on a case-by-case basis.

Hose and pad material:	PU; free of latex, heavy metals, and phthalates.
Ambient temperature in operation:	10 °C to 30 °C
Relative humidity:	Approx. 30 % to 70 %
Transport and storage temperature:	3 °C to 60 °C
Air pressure:	700 to 1060 hPa

Please refer to the corresponding brochures and price lists for any further information you require on the HICO water pads.

- Five-castor base, see section 4.2.3 (optional accessory) REF: 590002
- Clamp holder REF: 592900
- Equipotential bonding cable 1 m (optional accessory)
REF: 592905
- Sanosil (disinfectant solution) REF 830111
- Sanosil test strips (to determine the Sanosil content) REF 830112
- Female/male drain hose coupling (optional accessories; use only to drain the HICO PU pads) REF 550077/ 550078
- Female/male drain hose coupling SP (optional accessories; use only to drain the HICO PU pads SP) REF 550177 / 550178.

12 Guidelines and manufacturer's declaration

Guidelines and manufacturer's declaration - electromagnetic emissions

Tables for medical electrical equipment, general information:


Table 1

Guidelines and manufacturer's declaration - electromagnetic interference		
<p>The HICO-Aquatherm 660 is designed for operation in the electromagnetic environments listed in the tables and text of these instructions for use. The customer or user of the unit or system should ensure that the unit is used in an appropriate environment.</p>		
Electrical interference measurements	Agreement	Electromagnetic environment - guidelines
HF emissions according to CISPR 11	Group 1	The HICO-Aquatherm 660 uses RF energy exclusively for its internal functions. Therefore, its RF emission level is very low, and it is unlikely that it will interfere with nearby electronic devices.
HF emissions according to CISPR 11	Class B	
Emission of harmonics according to IEC 61000-3-2	(IEC 60601-1-2 Table 2) Class A	
Emission of voltage fluctuations/flicker according to IEC 61000-3-3	Agrees	The HICO-Aquatherm 660 is designed for use in facilities other than residential areas and in facilities that are directly connected to a public power supply that also supplies residential buildings.

Table 2

Guidelines and manufacturer's declaration – Electromagnetic immunity			
The HICO-Aquatherm 660 is designed for operation in an electromagnetic environment like the one listed below. The customer or user of the HICO-Aquatherm 660 should ensure that the device is used in such an environment.			
Immunity tests	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) according to IEC 61000-4-2	±8 kV contact discharge ±15 kV air discharge	±8 kV contact discharge ±15 kV air discharge	Floors should be wood, concrete, or ceramic tile. If the floor is covered with a synthetic material, then the relative humidity must be at least 30 %.
Electrical fast transient (EFT) / bursts according to IEC 61000-4-4	±2 kV for mains cables ±1 kV for input and output lines	±2 kV for mains cables Not applicable	The quality of the power supply voltage should correspond to that of a typical commercial or hospital environment.
Impulse voltage/surges according to IEC 61000-4-5	±1 kV voltage outer conductor-outer conductor ±2 kV voltage outer conductor-earth	±1 kV differential mode voltage ±2 kV common mode voltage	The quality of the power supply voltage should correspond to that of a typical commercial or hospital environment.
Voltage dips, short interruptions, and voltage variations according to IEC 61000-4-11	<5 % U_T (>95 % dip in U_T) for ½ cycle 40 % U_T (60 % dip in U_T) for 5 cycles 70 % U_T (60 % dip in U_T) for 25 cycles <5 % U_T (>95 % dip in U_T) for 5 sec	Voltage dips: 0 % U_T for 0.5 cycle (1 phase) 0 % U_T for 1 cycle 70 % U_T for 25/30 cycles (50/60 Hz) Voltage interruption: 0 % U_T for 250/300 cycles (50/60 Hz)	The quality of the power supply voltage should correspond to that of a typical commercial or hospital environment. If the user of the HICO-Aquatherm 660 requires continued operation during interruptions of the power supply, then we recommend supplying the HICO-Aquatherm 660 with power from an uninterruptible power supply or a battery.
Power frequency magnetic field (50/60 Hz) according to IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical commercial or hospital environment.
Comment: U_T is the alternating power supply voltage prior to application of the test level.			

Table 4

Guidelines and manufacturer's declaration – Electromagnetic immunity			
The HICO-Aquatherm 660 is designed for operation in an electromagnetic environment like the one listed below. The customer or user of the HICO-Aquatherm 660 should ensure that the device is used in such an environment.			
Immunity tests	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Conducted RF interference according to IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz 6 Vrms ISM and amateur bands	3 Vrms 150 kHz to 80 MHz 6 Vrms ISM and amateur bands	Portable and mobile radio equipment should be used no closer to the HICO-Aquatherm 660 and its power cables than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance: $d = 1.2\sqrt{P}$
Radiated RF interference according to IEC 61000-4-3	(IEC 60601-1-2 Table 4) 3 V/m 80 MHz to 2,7 MHz (Proximity fields for wireless communication equipment IEC 60601-1-2 Table 9) 380 - 390 MHz 27 V/m; PM 50 %; 18 Hz 430 - 470 MHz 28 V/m; (FM ±5 kHz, 1 kHz sine) PM; 18 Hz 11 704 - 787 MHz 9 V/m; PM 50 %; 217 Hz 800 - 960 MHz 28 V/m; PM 50 %; 18 Hz 1700 - 1990 MHz 28 V/m; PM 50 %; 217 Hz 2400 - 2570 MHz 28 V/m; PM 50 %; 217 Hz 5100 - 5800 MHz 9 V/m; PM 50 %; 217 Hz	(IEC 60601-1-2 Table 4) 3 V/m 80 MHz to 2,7 MHz (Proximity fields for wireless communication equipment IEC 60601-1-2 Table 9) 380 - 390 MHz 27 V/m; PM 50 %; 18 Hz 430 - 470 MHz 28 V/m; (FM ±5 kHz, 1 kHz sine) PM; 18 Hz 704 - 787 MHz 9 V/m; PM 50 %; 217 Hz 800 - 960 MHz 28 V/m; PM 50 %; 18 Hz 1700 - 1990 MHz 28 V/m; PM 50 %; 217 Hz 2400 - 2570 MHz 28 V/m; PM 50 %; 217 Hz 5100 - 5800 MHz 9 V/m; PM 50 %; 217 Hz	$d = 1.2\sqrt{P}$ 80 MHz to 800 MHz $d = 2.3\sqrt{P}$ 800 MHz to 2.5 GHz Where P is the output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). The field strength from a stationary radio transmitter, as determined by an electromagnetic site survey ^a , should be less than the compliance level ^b in all frequency ranges. Interference may occur in the vicinity of equipment marked with the following symbol. 

NOTE 1: At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. The propagation of electromagnetic waves is affected by the absorption and reflection from structures, objects, and people.


^a Field strength from fixed transmitters such as base stations for radio (cellular/wireless) telephones and land mobile radios, amateur radio, AM/FM radio stations, and TV stations cannot be predicted theoretically with accuracy. To determine the electromagnetic environment of a stationary transmitter, an electromagnetic site survey should be considered. If the measured field strength in the location in which the HICO-Aquatherm 660 is used exceeds the compliance level listed above, then the HICO-Aquatherm 660 should be monitored to verify normal operation. If abnormal performance is observed, additional measures might be necessary, such as re-orienting or relocating the HICO-Aquatherm 660 or the use of a shielded location with higher RF shielding effectiveness and filter attenuation.

^b The field strength should be less than 3 V/m over the frequency range of 150 kHz to 80 MHz.

Table 6

Recommended separation distance between portable and mobile RF communications equipment and the HICO-Aquatherm 660			
The HICO-Aquatherm 660 is designed for operation in an electromagnetic environment in which RF interference is controlled. The customer or the user of the HICO-Aquatherm 660 can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the HICO-Aquatherm 660 depending on the power output of the communications equipment as indicated below.			
Output power of the transmitter W	Separation distance depending on the transmitter frequency m		
	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2.5 GHz
	$d = 1.2\sqrt{P}$	$d = 1.2\sqrt{P}$	$d = 2.3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23
For transmitters whose maximum output power rating is not listed in the table above, the distance can be determined using the equation shown in the corresponding column, where P is the maximum output power rating of the transmitter in watts (W) according to the manufacturer of the transmitter.			
NOTE 1: At 80 MHz and 800 MHz, the higher frequency range applies.			
NOTE 2: These guidelines may not apply in all situations. The propagation of electromagnetic waves is affected by the absorption and reflection from structures, objects and people.			

13 Quick Start Guide

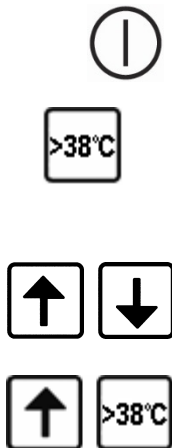

- Connect the unit to the mains supply.
- Connect the water pad to the unit.
- Check the water level on the unit.
- Switch on the unit using the power switch and watch the automatic function test.
- If the nominal temperature setting is $> 38\text{ }^{\circ}\text{C}$ when switching on the unit, then an alarm will be emitted. Acknowledge and start by pressing the release key.
- Set the temperature with the arrow keys.
- For temperatures above $38\text{ }^{\circ}\text{C}$, press the arrow key and the release key at the same time.
- Depending on the application, place the water pad under or on top of the patient.
- Monitor the body temperature of the patient.
- Monitor the water level and water flow on the unit.
- In case of continuous operation, perform a manual function test once every day by pressing the “Function test” key.
- Acoustic alarms of medium priority (“WATER LEVEL!?” and “TEMP.DIFF $> 1^{\circ}\text{C}$ ”) can be interrupted for 10 minutes using the “Mute audio” key.
- All other acoustic alarms of medium priority cannot be interrupted. Switch off the unit using the power switch (16).

▲WARNING

There is a risk of the patient becoming overheated or undercooled.

- ▶ Monitor the patient's body temperature when using the unit and the water pad on the patient.

▲CAUTION

Do not start the unit in the following cases:

- ▶ The display has failed.
- ▶ Individual segments of the temperature display have failed (temperature can no longer be read properly).
- ▶ The yellow error light (13) is continuously lit or does not light up at all (functional test).
- ▶ The alarm signal tone continues to sound or does not sound at all (functional test).
- ▶ The unit does not respond when you press a key.
- ▶ The unit does not respond as described in section 6.2.3 "Functional test" when switching on the unit or during a function test.